

Minimum Standard for Portable
Gaseous, Oxygen Equipment

NOTICE

Changes in this reaffirm are format/editorial only.

1. SCOPE:

This standard is intended to apply to that portable compressed gaseous oxygen equipment used for the administration of supplementary and/or first aid oxygen to one or more occupants of either private or commercial transport aircraft.

This standard is applicable to the following types of portable oxygen equipment:

- a. Continuous flow;
- b. Demand flow;
 1. Straight demand
 2. Diluter demand
 3. Pressure demand
- c. Combination continuous flow and demand flow.

2. PURPOSE:

This standard defines the general minimum standards for the design specifications, testing and packaging of portable oxygen breathing equipment, incorporating an integral compressed gas oxygen supply (Refer to AS1303 for Portable Chemical Oxygen).

SAE Technical Standards Board Rules provide that: "This report is published by SAE to advance the state of technical and engineering sciences. The use of this report is entirely voluntary, and its applicability and suitability for any particular use, including any patent infringement arising therefrom, is the sole responsibility of the user."

SAE reviews each technical report at least every five years at which time it may be reaffirmed, revised, or cancelled. SAE invites your written comments and suggestions.

Copyright 2000 Society of Automotive Engineers, Inc.
All rights reserved.

Printed in U.S.A.

TO PLACE A DOCUMENT ORDER:
SAE WEB ADDRESS:

(724) 776-4970
<http://www.sae.org>

FAX: (724) 776-0790

SAE AS1046 Revision B

3. REFERENCES:

The requirements set forth in AS861 shall be considered as part of this standard, except that in event of conflict, this standard shall take precedence.

3.1 Applicable Documents:

SAE

AIR825B	Oxygen Equipment for Aircraft
AS861	Minimum General Standards for Oxygen Systems
AIR1059A	Transfilling & Maintenance of Oxygen Cylinders
AS1065	Quality and Serviceability Requirements for Aircraft Cylinder Assemblies
AIR1176	Oxygen System and Component Cleaning and Packaging
AS1219	Aircraft Oxygen Replenishment Coupling for Civil Transport Aircraft
AS1224	Continuous Flow General Aviation Oxygen Masks
AS1248	Minimum Standard for Oxygen Pressure Reducers
AS303	Portable Chemical Oxygen
AS8010A	Aviators Breathing Oxygen Purity Standard
AS8025	Passenger Oxygen Mask
AS8026	Crewmember Oxygen Demand Mask for Transport Category Aircraft

Other

MIL-P-7105	Pipe Threads, Taper, Aeronautical National Form, Symbol ANPT
MIL-S-7742	Screw Threads Standard, Aeronautical
MIL-O-27210	Oxygen, Aviator's Breathing, Liquid and Gas
MIL-T-27730	Tape, Antiseize, Tetrafluoroethylene, with Dispenser
FAR PART 21	Certification Procedures for Products and Parts
FAR PART 25	Airworthiness Standards Transport Category Airplanes
FAR PART 23	Airworthiness Standards Normal, Utility and Acrobatic
FED-STD-595	Federal Standard Colors
CGA S-1.1	Pressure Relief Device Standards - Part 1 Compression Gas Association
TARIFF BOE 6000	Hazardous Materials Regulations of the Department of Transportation (DOT) 49 CFR 170
TSO-C89	Oxygen Regulators, Demand

4. REQUIREMENTS:

4.1 Detail Requirements:

Each portable unit shall consist of the following basic components:

- a. Oxygen cylinder
- b. Oxygen pressure reducer and/or flow regulator with necessary accessories
- c. Mask(s)
- d. Harness (optional)
- e. Overall container (optional)

4.2 Oxygen Cylinder:

The oxygen cylinder shall conform to Department of Transportation (DOT) Specifications 3A or 3AA or to any other DOT specifications for transportable cylinders for oxygen service. The cylinder shall be permanently marked to show the applicable DOT specification number, service pressure and most recent test date. Prior to assembling components to the cylinder, it shall be cleaned to those levels specified in AIR1176.

4.2.1 Filling Pressure: The filling pressure shall be prominently shown for the benefit of the user by a stencil, label or other durable marking and shall not exceed the DOT service pressure rating stamped near the neck of the cylinder. If the equipment meets the requirements for 10% overcharging as indicated by a plus sign (+) following the test date marking on the cylinder, this shall be shown on the stencil or other marking. For example, a cylinder manufactured to specification DOT 3AA 1800 will be marked "MAX. PRESSURE 1980 PSIG @ 70°F (13.65 MPa @ 21.1°C)". This is equivalent to the noted service pressure x 110%.

4.2.1.1 Gas: The cylinder shall be filled with aviator's breathing oxygen conforming to MIL-O-27210 or AS8010.

4.2.2 Size and Shape: The dimensions and shape of the cylinder shall be as required by, or acceptable to, the purchaser.

4.2.2.1 Protrusions: External tubing or other provisions that might be used as carrying or supporting handles must be designed to safely withstand the loads which might be imposed on them.

4.2.3 Capacity: The gaseous volume of oxygen in liters (dm³) NTPD, contained in the cylinder when charged to its rated pressure shall be indicated on the cylinder by stencil, label or other durable marking. For example, an acceptable marking is "CONTAINS XXXX LITERS, NTPD, WHEN CHARGED TO XXXX PSIG", or "CONTAINS XXXX dm³ NTPD, WHEN CHARGED TO XXXX MPa". NTPD indicates Normal Temperature and Pressure, Dry; that is, at 21°C (70°F) and 760 mm Hg (0.101325 MPa).

SAE AS1046 Revision B

4.2.4 Duration: The rated altitude and the duration of oxygen in the cylinder when filled to its rated pressure shall be indicated by a stencil, label or other durable marking. It shall show the duration of the supply when used at its rated altitude by one person. For continuous flow types of portable equipment, the duration shall be calculated based on the average flow at the rated altitude. For demand, diluter demand, and pressure demand the duration shall be based on a minute volume of 20 L (dm³) BTPS*, and using an average oxygen-air mixing ratio.

By nature, demand systems vary greatly in oxygen usage because of variations in user's vital capacity, rate of exercise, etc. Therefore, the above-rated duration should be considered average only and shall be noted as "average duration".

*BTPS - Body temperature, pressure, saturated (37°C, ambient pressure, saturated with water vapor at 37°C. p_{H₂O} at 37°C = 47 mm Hg (6.27 kPa))

4.2.5 Color: Color of the cylinder and other components shall be optional with the purchaser. Unless otherwise specified, cylinders shall be painted green per color No. 14187 of FED-STD-595.

The cylinder shall be prominently and durably marked "AVIATOR'S BREATHING OXYGEN".

4.2.6 Cylinder-to-Regulator Attachment: The attachment of the regulator, valve, or other component to the oxygen cylinder may be by one of the following:

- a. Taper pipe threads conforming to MIL-P-7105 and using as a thread, anti-seize, Teflon® tape conforming to MIL-T-27730
- b. Straight threads conforming to MIL-S-7742 with a gasket seal; the gasket material shall be compatible for use with high-pressure oxygen

4.3 Regulator:

The regulator shall control the delivery of oxygen to the user(s) either through a continuous-flow metering device, through a demand regulator, or both. The following accessories shall be deemed a part of the regulator, although they may not all be integral portions of a single unit, but may be arranged as separate components interconnected.

- a. ON-OFF valve
- b. Cylinder contents indicator (pressure gage)
- c. High pressure safety relief device
- d. Low pressure relief valve
- e. Filler fitting
- f. One or more continuous-flow outlets and/or a demand type regulator
- g. Flow indicator (optional)

SAE AS1046 Revision B

4.3.1 Regulator Performance:

- 4.3.1.1 Pre-Set Continuous-Flow Type: Unless otherwise specified by the purchaser, the mass flow of oxygen from each outlet shall be such that when used in combination with the mask recommended by the manufacturer (or selected by the user), the combination will deliver to the user sufficient oxygen to maintain the minimum tracheal oxygen partial pressure or mass flow rate specified in the appropriate paragraph(s) of FAR Part 25.1443, or FAR Part 23.1443, at the altitude(s) stipulated by the manufacturer. The highest altitude at which this requirement is met shall be clearly indicated by a permanent stencil, decal, label or other means as the maximum recommended altitude.
- 4.3.1.2 Adjustable Continuous Flow Type: The regulator may be provided with a means for varying the flow of oxygen either by adjustment of the regulator, adjustment of the constant flow outlet, or other means. When such adjustment is provided, its use shall be clearly explained in a permanent stencil, label, or other means. Unless otherwise specified by the purchaser, the flow of oxygen shall be adequate (when used in combination with the mask recommended by the manufacturer or selected by the user) to maintain a minimum tracheal oxygen partial pressures or mass flow rate specified in the appropriate paragraph(s) of FAR Part 25.1443, or FAR Part 23.1443 at the altitudes stipulated by the manufacturer.
- 4.3.1.3 Automatic Continuous Flow Type: The regulator shall be provided with an automatic mechanism that will vary the flow of oxygen in accordance with altitude. Its operation shall be clearly explained in a permanent stencil, label, or other means. Unless otherwise specified by the purchaser, the flow of oxygen shall be adequate (when used in combination with the mask recommended by the manufacturer or selected by the user) to maintain the minimum tracheal oxygen partial pressures specified in the appropriate paragraph(s) of FAR Part 25.1443, or FAR Part 23.1443 at the altitudes stipulated by the manufacturer.
- 4.3.1.4 Demand Type: When a demand regulator is included in the equipment, either alone or in combination with one or more continuous flow outlets, the demand regulator shall deliver oxygen from the regulator in response to the inspiratory effort (draft) of the user. The demand regulator shall meet the requirements of FAA TSO-C89.
- 4.3.1.5 Diluter-Demand Type: In response to the inspiratory effort of the user, the diluter-demand regulator shall deliver a mixture of air and oxygen. The concentration of oxygen in the mixture delivered to the mask shall be not less than that required to maintain a minimum tracheal partial pressure of oxygen of 122 m Hg (16.3 kPa) at inspiratory flow rates of 10 to 120 LPM-BTPS (dm^3/min) within the altitude range stipulated by the manufacturer. Where the equipment is to be used for passengers the tracheal partial pressures and flow rates must conform to FAR 25.1443(C). The altitude to which the regulator will perform this function shall be clearly indicated by means of a stencil, label, or other durable marking.

SAE AS1046 Revision B

- 4.3.1.6 Pressure-Demand Type: The pressure-demand regulator shall deliver oxygen to the mask at a positive (above atmospheric) pressure at those altitudes or under other conditions where 100% oxygen is required. Such a pressure shall be sufficient to:
- Provide protection against smoke during firefighting by precluding inward mask leakage of the ambient atmosphere; and/or
 - Partially compensate for reduced barometric pressure at altitudes at which 100% oxygen at ambient atmospheric pressure is inadequate for physiological needs.

The pressure demand regulator shall meet the requirements of FAA TSO-C89.

- 4.3.2 ON-OFF Valve: An ON-OFF valve shall be provided to control the delivery of oxygen from the cylinder. The valve may be one of the following:
- A high pressure valve between the cylinder and the pressure reducer/regulator
 - A pressure reducer/regulator mechanism designed to serve as both an ON-OFF valve and a regulating control
 - A low pressure valve on the downstream side of the pressure reducer
- 4.3.2.1 High Pressure Valve: The valve shall isolate the cylinder contents from all parts of the regulator except the cylinder contents gauge and the high pressure safety relief device. The filler valve may be on either side of the high pressure shut off valve.
- 4.3.2.2 Valve-Regulator Combination: A means shall be provided for mechanically controlling the regulating valve for the purpose of either preventing flow from passing the regulating valve or allowing flow to pass through the regulator and allowing it to function simultaneously as a pressure reducer.
- 4.3.2.3 Low-Pressure Valve: A low pressure valve on the downstream side of the pressure reducing regulator shall, by stopping the discharge of gas, cause the pressure reducer valve to close and prevent further entry of gas from the cylinder to the outlets.
- 4.3.3 Valve Design, Construction, and Materials: The requirements and recommendations of AIR825 shall be considered in the design of valves. Valve seats, seals, or other nonmetallic materials shall be compatible for use with oxygen at the maximum working pressure and temperature anticipated. (See also AS1248.)
- 4.3.4 Valve Control: The valve control shall be clearly and durably marked to indicate the direction of movement to open or close the valve. The valve control may be of the rotating knob, rotating lever, or "push-pull" type. Rotating type controls shall be of ample size, properly contoured, and shall operate with a torque not exceeding 1.7 Nm (15 in lb). "Push-Pull" type controls shall require not more than 44.5N (10 lb) of force to either open or close the valve.

SAE AS1046 Revision B

- 4.3.5 Cylinder Contents Indicator: The indicator shall at all times (regardless of whether the on-off valve is open or closed) indicate (in psi, unless otherwise specified) the pressure existing in the cylinder. If so specified by the customer, the indicator may show the maximum filling pressure and the pressure at which the cylinder should be refilled. The use of the color red in bands to signify fill levels shall be avoided.
- 4.3.6 High Pressure Safety Device: The safety device shall be of a type approved by the Bureau of Explosives and shall comply with the requirements of CGA Pamphlet S-1.1. It shall service to release the contents of the cylinder at some pressure not greater than 1.67 times the DOT rated service pressure of the cylinder. The outlet of the device shall be designed to minimize the propulsive effects of the escaping gas. It shall be safety wired where feasible.
- 4.3.7 Low Pressure Relief Valve: The low pressure relief valve shall release from the reduced pressure area of the regulator any pressure in excess of that which can be safely contained, or in excess of that which will permit safe performance of the regulator. The valve shall reclose after release of excess pressure.
- 4.3.8 Continuous Flow Oxygen Connection: The style and type of connection shall be optional with the purchaser. On connections used with a pre-set regulator, the connection shall be marked to indicate the oxygen flow rate and rated altitude. Color coding (or other equivalent means), explained by a durable decal or label, is acceptable. The connection shall be designed to permit easy coupling by a cabin attendant.
- 4.3.9 Filler Fitting: The equipment shall be provided with a fitting through which the oxygen cylinder can be refilled from a source of gaseous oxygen under adequate pressure. The fitting shall be in accordance with Item A of Fig. 1. The filler fitting shall incorporate a filter of 125 μm nominal or better particle retention. The fitting shall be protected against damage or contamination by a removable cap or equivalent means. As an alternate, the filler fitting shall be in accordance with AS1219.
- 4.4 Flow Indicator:
- If required by the purchaser, an indicator may be provided to indicate to the user that oxygen is being delivered to the dispensing equipment.
- 4.5 Harness:
- When and as specified by the purchaser, the equipment may be provided with a harness whereby the equipment can either be conveniently carried or worn, either by a crew member or by a passenger using the equipment. When furnished with a shoulder strap, the equipment should also be provided with a waist belt or some type of restraint to minimize uncontrolled swinging of the unit when worn by an ambulatory crew member or passenger. Choice of material, color and design detail of the harness shall be at the option of the purchaser.

SAE AS1046 Revision B

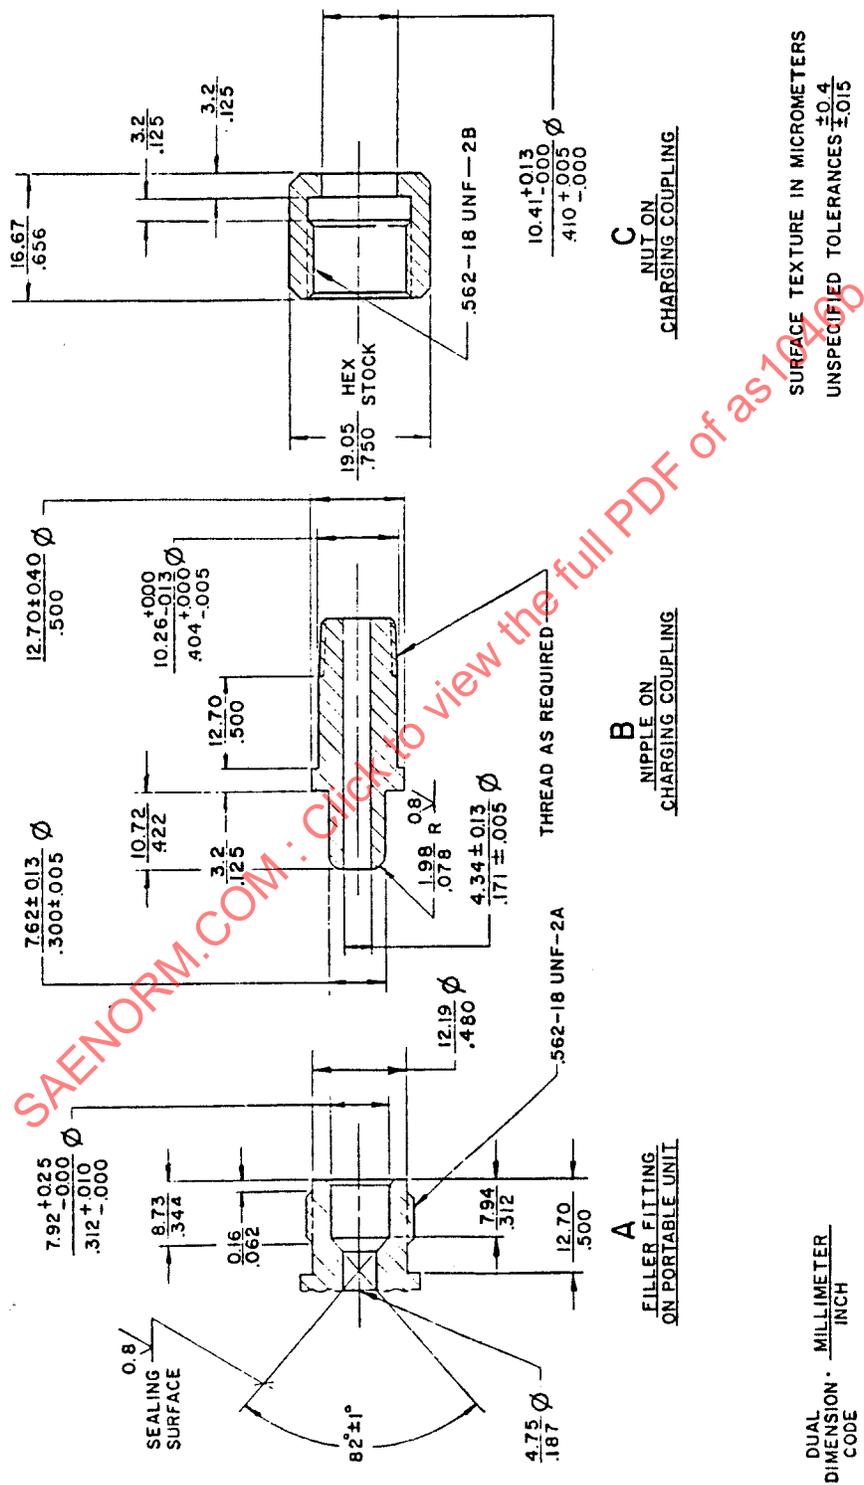


FIGURE 1